


Aliastm

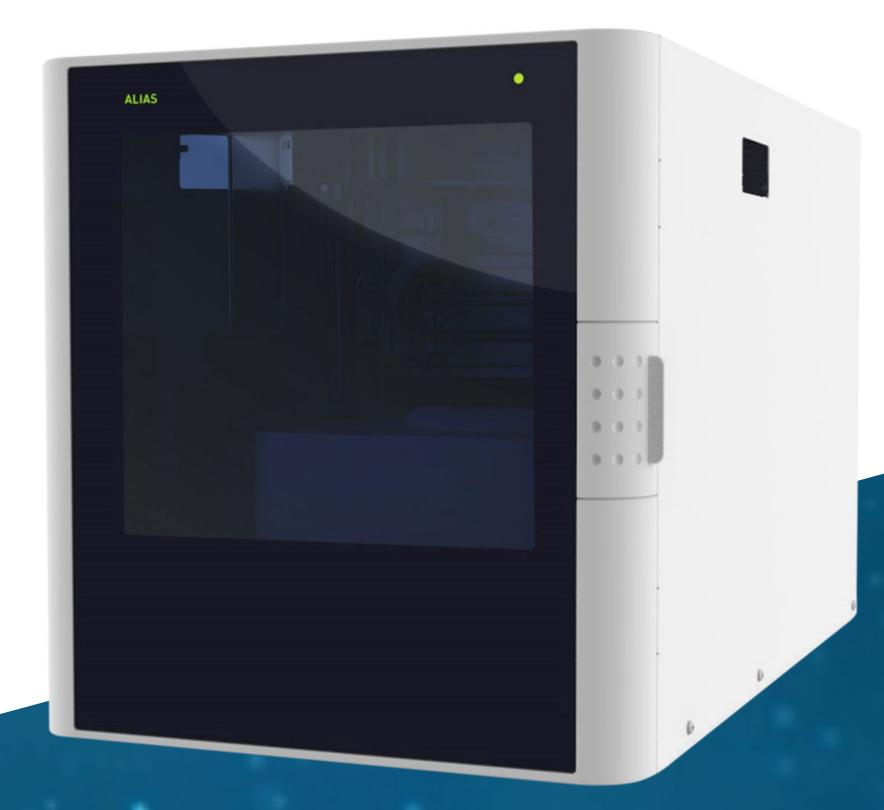

Generic autosampler for liquid samples

> sparkholland.com


Better Sample Care.


Alias

The perfect workhorse for your HPLC system

Generic autosampler for liquid samples

Alias™ is a generic autosampler for applications like HPLC and LC-MS, using proven injection technology with fast injection and wash cycles. Designed to fit any system for any application. Multi-solvent needle wash virtually eliminates carry-over. Alias™ handles well plates and sample vials, either open or sealed, and provides true 4°C sample cooling. Its compact, stackable design and unrivalled performance make the Alias™ autosampler the perfect workhorse for your (U) HPLC system.

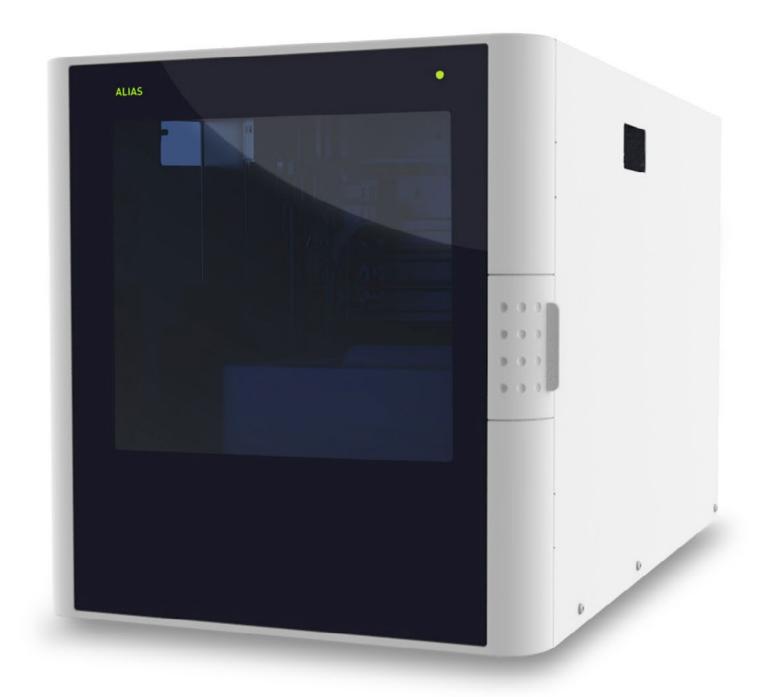

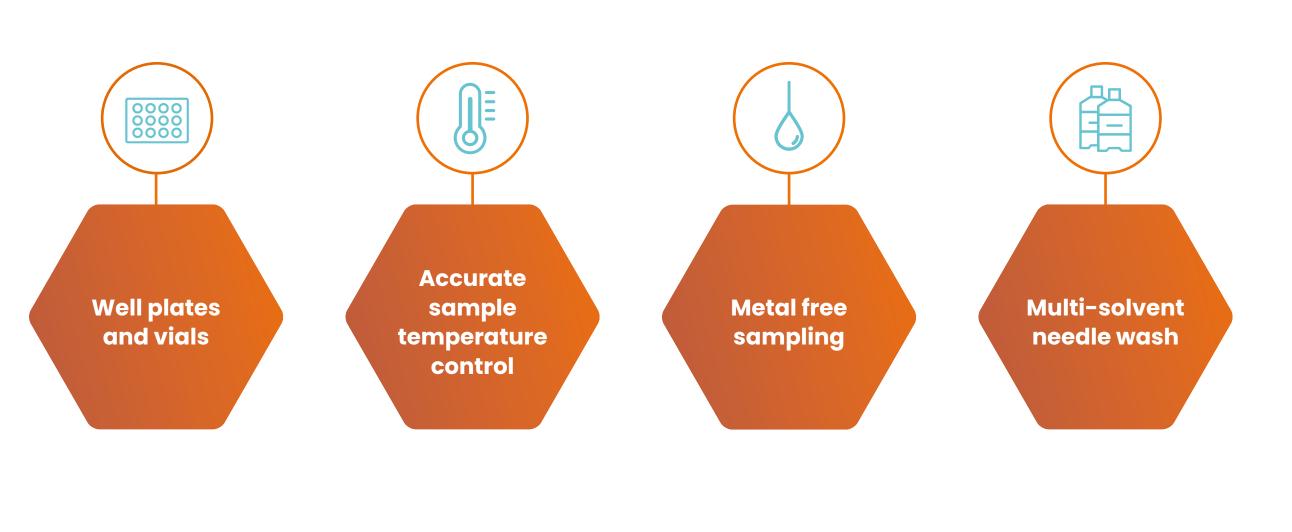





Alias™ UHPLC

Alias™ is also available as a UHPLC compatible version permitting injection into UHPLC systems operated at pressures as high as 18,000 PSI. A special injection routine has been developed to eliminate influence of sample loop decompression on injection performance. The UHPLC version can also be equipped with sample cooling.

Alias™ Prep LC

A special modification for large volume injections turns the Alias™ into a perfect injector for your preparative LC system. The Alias™ Prep version holds 24 vials of 10 mL and uses a 2.5 mL syringe. Needles, tubing and sample loop have larger capacity and allow rapid injection of sample volumes up to 10 mL.

Features and options

- Metal free sampling with silica-coated steel needle and PEEK valve (option)
- Reagent addition and mix capabilities for derivatization, dilution, internal standard addition
- Optional 6-port solvent selection valve (SVV) for extended selection of reagents for needle wash and reagent addition (option)
- Integrated Stream Switching (ISS): optional extra high pressure 6-port switching valve for column switching or other stream switching applications up to 18,000 PSI
- Quick-fit injection valve for fast service









Specifications

	ALIAS	ALIAS UHPLC
Injection modes	Full-loop Partial loop-fill µL-pick-up	Pressure Assisted Sample Aspiration using ~10 PSI sample headspace pressure to avoid air bubbles in sample lines.
Injection volume	Programmable from 0 μl – 9999 μL 1 μL increments	Max injection volume depends on installed sample loop and injection mode
Injection precision	Full-loop injection < 0.3% RSD Partial loop-fill < 0.5% RSD µL-pick-up < 1.0% RSD	For injection volumes > 5 µL
Sample viscosity	0.1 - 5 cP	
Injections per vial/well	Max 9	
Syringe volume	500 µL standard 250, 1000 and 2500 µL optional	
Needle wash Inside and outside needle wash with drying. Wash can be programmed between injections and between vials/wells.	1 solvent 5 additional wash solvents	Programmable volume from a 250 µL wash reservoir SSV option required
Injection cycle time	60 seconds	« 20 seconds, with typical 10 μL injection (loop fill with rinse buffer)
Valve switching time	60 msec	
Wetted parts	SS316, PTFE, TEFZEL, VESPEL, glass, For Bio-kit option: PEEK and coated-steel (needle) instead of SS316	
Carry-over	0.05% with standard washTypically < 0.01% with extra wash	"zero carry-over" can be accomplished with ALIAS™ wash capabilities
Sample capacity	Microtiter plates: 2 Vials: 2x 48 (1.5 mL) or 2x 12 (10 mL) - optional	Microtiter plates according to SBS standards. 96-well high and low and 384-well.
Maximum vial/MTP height	47 mm	including cap
Sample cooling Factory installed option (Peltier technology)	Minimum: 4°C ± 2°C Maximum: ambient temp -3°C	Measured as air temperature in sample compartment for maximum ambient temperature 25°C and maximum humidity 80%

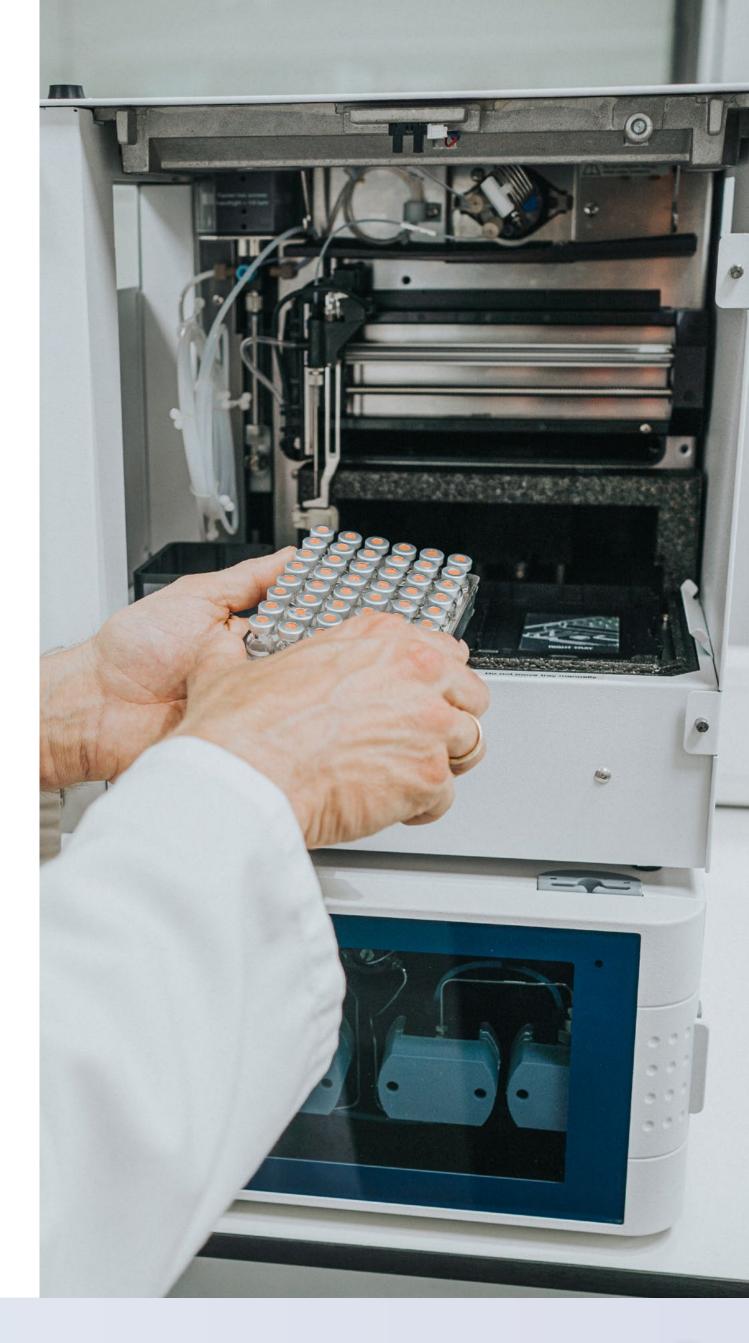







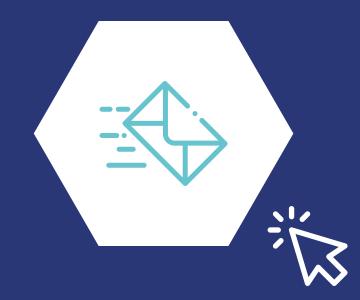

Get in touch

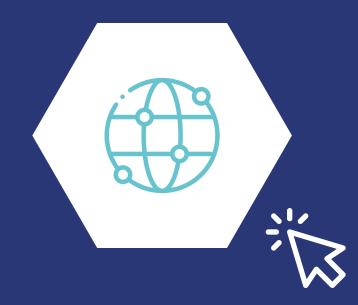

Visit our website

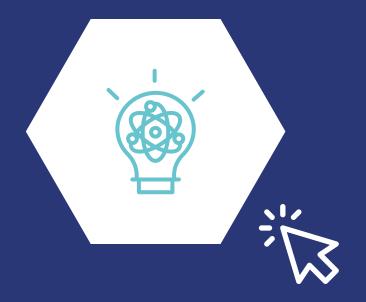

Our technologies

